

Investigation on interaction of radiofrequency waves (microwaves) with saphenous veins

Karthik Baskar ^{1*}, Pavithra Krishnamoorthy ², Nehrujee Vishalinee ¹,
Padmavarshini Sivakumar ¹, Anita ¹, Varshini Karthik²

¹ Assistant Professor Department of Biomedical Engineering, SRM Institute of Science and Technology, Kattankulathur

² Head of the Department in-charge Department of Biomedical Engineering, SRM Institute of Science and Technology, Kattankulathur

Abstract

Varicose veins contract when heated through microwave ablation. Heat application through microwave ablation, the collagen tends to regain its elasticity. In this paper, we propose simulation of the varicose vein with a wearable micro strip patch antenna. ANSYS HFSS 17.2 is an electromagnetic finite element method solver. The phantom model of human skin with normal vein and varicose vein with a wearable micro strip patch antenna was designed using this software. The wearable micro strip patch antenna is designed so that this approach is minimally invasive. The wearable micro strip patch antenna is modelled with a resonant frequency of 9.8 GHz. The temperature of about 45°C is proposed as the treatment for varicose vein.

Keywords: SSV-Small Saphenous Vein; SAR-Specific Absorption Rate; S-Seconds; W/Kg-Watts per Kilogram; GHZ-Gigahertz; W-Watts; Mm-Millimetre; °C-Degree Celsius.

1. Introduction

Varicose vein is an aberrance of a superficial vein. Varicose veins patients are present in 15% of men and 25% of woman. The commonness of this disease is due to family history, female hormones, arterial venous connections, physiological and biochemical stress. Varicose vein is generally treated surgically. The medical procedure takes forever and ever and large abrasion size. Varicose veins are caused in weak or damaged veins. After arteries and capillaries pass oxygenated blood throughout the body, veins return the blood to the heart, the veins in legs must work against gravity to do this. Hence there are valves inside the veins that open and let the blood flow through, and then they close to keep blood from flowing backwards. If these valves are weakened or damaged, blood can flow back and pool in the veins, this causes the veins to swell. Habitually, the walls of these veins are elastic (stretchy). When the valve flaps of these veins separate, blood can flow backward through the valves.

1.1. Effect of collagen on varicose veins

Collagen is the connective tissue that gives structural support to your body by binding cells or tissues together. Collagen is a protein that accounts for over one-fourth of all the protein in your body. More importantly, collagen is responsible for maintaining the elasticity and strength of your blood vessels. An imbalance between the synthesis of collagen I and collagen III explains the lack of elasticity of varicose veins.

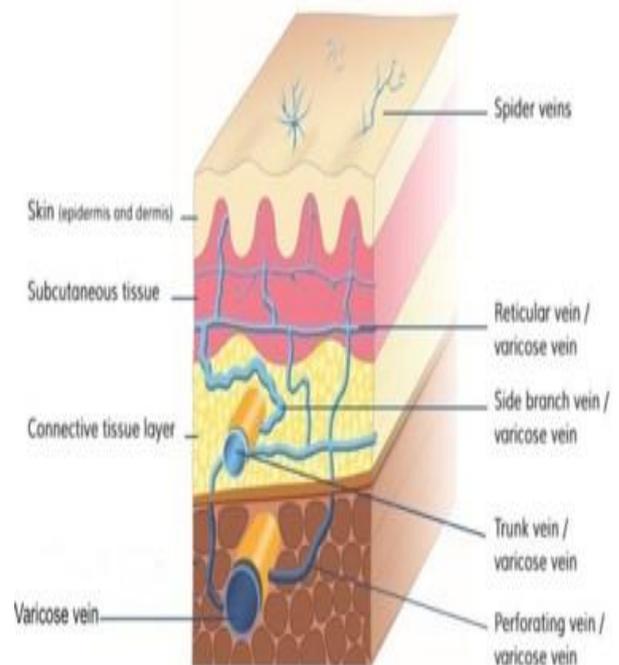


Fig. 1: Structure of Varicose Veins.

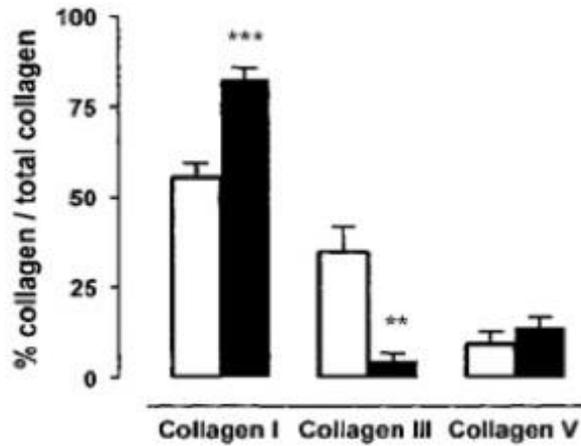


Fig. 2: Effect of Collagen.

2. Methodology

2.1. Modelling of varicose veins

The phantom model of varicose vein is designed using ANSYS HFSS 17.2 software. The cylindrical model has been designed for the human skin layers with normal and varicose veins. In this model, the blood vessel is the Small Saphenous vein (SSV) which is present between the hypodermis and subcutaneous tissue and a tributary of the SSV is present in the dermis layer of the skin. The dielectric properties of skin dry, blood vessel and subcutaneous tissue have been created in ANSYS HFSS 17.2 software for epidermis, dermis and hypodermis.

Table 1: Dielectric Properties of Skin Dry, Blood Vessel and Subcutaneous Tissues

3	PROPERTIES	SKIN DRY	BLOOD VESSEL	SUBCUTANEOUS TISSUE
1.	Relative permittivity	33.367	35.533	4.779
2.	Relative permeability	1	1	1
3.	Bulk conductivity	5.6172 S/m	0.42899 S/m	6.5686 S/m
4.	Dielectric loss tangent	0.38797	0.20687	0.42447
5.	Measured frequency	7.8 GHz	7.8 GHz	7.8 GHz
6.	Mass density	1050 kg/m ³	994 kg/m ³	1035 kg/m ³

2.2. Wearable micro strip patch antenna

Micro strip patch antenna is becoming eventually used because they are imprinted directly onto a circuit board. The antenna which is used for our purpose is wearable micro strip patch antenna. The patch antenna, micro strip transmission line and ground plate are made up of high conductivity metal (typically copper). The main advantage of wearable antennas is that they are drafted as elements of clothing able to transmit or receive wireless signals. The wearable antenna system plays an important role in many fields, including tracking and exploration. The wearable micro strip patch antenna is designed with various resonant frequencies such as 3.3 GHz, 6.4 GHz, 9.8 GHz and 14 GHz.

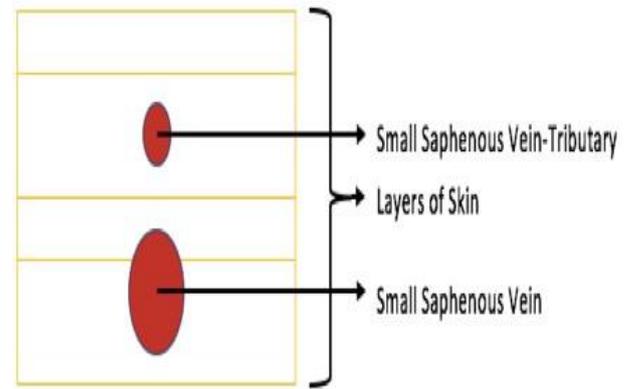


Fig. 3: Design of Varicose Vein-1.

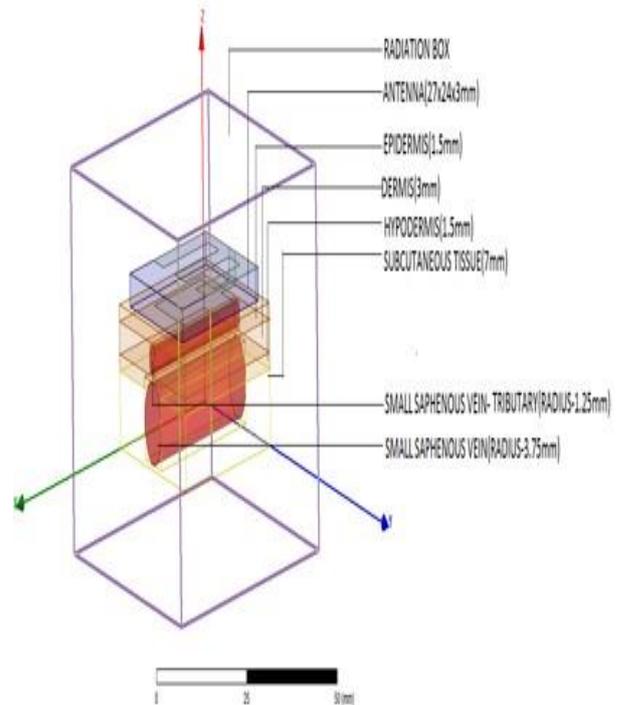


Fig. 4: Design of Varicose Vein-2.

Table 2: Design Parameters of Normal & Varicose Vein

S. No.	LAYERS	PROPERTIES	NORMAL VEIN	VARICOSE VEIN
1.	Epidermis	Skin dry	1.5mm	1.5mm
2.	Dermis	Skin dry	1.5mm	1.5mm
3.	Tributary-SSV	Blood Vessel(Radius)	0.65mm	1.25mm
4.	Hypodermis	Skin dry	1.5mm	1.5mm
5.	Small Saphenous Vein	Blood Vessel(Radius)	4mm	3.75mm
6.	Subcutaneous Tissue	Subcutaneous Tissue	4mm	7mm

2.3. Design parameters of wearable microstrip patch antenna

1) Width (W)

The width of the patch is reckoned using the following formula, Equation 1 Width of the Patch

$$W = \frac{C_0}{2f_r} \sqrt{\frac{2}{\epsilon_r + 1}}$$

Where,

W = Width of the patch

C_0 = Speed of light

ϵ_r = value of the dielectric substrate

2) Effective Refractive Index:

The effective refractive index value of a patch is an important criteria in the making of a micro strip patch antenna. The radiations enrooted from the patch towards the ground travel through air and substrate this effect is known as fringing effect. Both the air and substrates have different dielectric values, therefore to account for this, we find the effective dielectric constant. The value of the effective dielectric constant (ϵ_{reff}) is calculated using the following formula,

Equation 2 Effective Refractive Index

$$\epsilon_{\text{reff}} = \frac{\epsilon_r + 1}{2} + \frac{\epsilon_r - 1}{2} \left[1 + 12 \frac{h}{W} \right]^{-1/2}, W/h > 1$$

Where,

ϵ_r = value of the dielectric substrate

h = height of the substrate

W = width of the substrate

3) Length (L)

Due to fringing effect, electrically the length of the antenna is increased by an amount of L . Therefore, the actual increase in length (L) of the patch is to be calculated using the following formula ,

Equation 3 Length of the Patch

$$L = \frac{C_0}{2f_r \sqrt{\epsilon_{\text{reff}}}} - 2\Delta L$$

4) Length (L_g) and Width (W_g) of Ground Plate

The length and width of a substrate are equal to that of the ground plate. The length of a ground plate (L_g) and the width of a ground plate (W_g) is calculated using the following equations, Equation 4 Length and width of Ground Plate

$$L_g = 6h + L$$

$$W_g = 6h + W$$

5) The width of the Microstrip Transmission Line

The width of Transmission line (TL) is given by the following formula,

Equation 5 Width of Transmission Line

$$TL = \frac{\lambda}{4} = \frac{\lambda_0}{4 \sqrt{\epsilon_r}}$$

2.4. Substrate

Generally, for micro strip antennas, the substrate's dielectric constants ranges from 2.2 to 12. Here we have chosen different cotton textiles like jean cotton, wash cotton, polycotton and certain cotton as substrates. The radiation parameters greatly depend on the substrate hence must be chosen carefully. The substrate which we have used is wash cotton. The properties of wash cotton are given in table 3.

2.5. Design of the micro strip patch antenna

The design of micro strip patch antenna comprises of the radiating patch, transmission line, substrate and the ground plate. The radiating patch is a two-dimensional structure constructed with the dimensions of 16.7mmx15mm with the property of Copper/Perfect E. The transmission line is a two-dimensional structure constructed with the dimensions of 5.15mmx3.1mm with the property of Copper/Perfect E. The substrate is a three-dimensional structure of the dimensions of 27mmx24mmx3mm with the properties of wash cotton. The ground plate is a two-dimensional structure with the properties of Copper/Perfect E. Different types of ground plates were tried for the antenna and the required frequency response was only obtained by etching the structure E in the ground plate. The wearable micro strip patch antenna has been designed for both saphenous veins (normal and varicose).

Table 3: Dielectric Properties of Substrate

S. No.	PROPERTIES	VALUES
1.	Relative permittivity	1.51
2.	Relative permeability	1
3.	Bulk conductivity	0
4.	Dielectric loss tangent	0.02
5.	Measured frequency	7.8 GHz
6.	Mass density	1500 kg/m ³

Table 4: Design Parameters of the Wearable Microstrippatch Antenna

S. No.	Design Properties	Dimensions
1.	Length of the patch	16.7mm
2.	Width of the patch	15mm
3.	Length of the substrate	27mm
4.	Width of the substrate	24mm
5.	Height of the substrate	3mm
6.	Width of transmission line	3.1mm

3. Analysis

In this study, we are analyzing all the parameters mentioned below: ● Specific Absorption Rate ● Temperature ● Time period for the radiation to occur ● Power level. The maximum temperature that a human body can resist is 45°C. We also use 45°C of temperature by varying the time period of radiation occurred in the body.

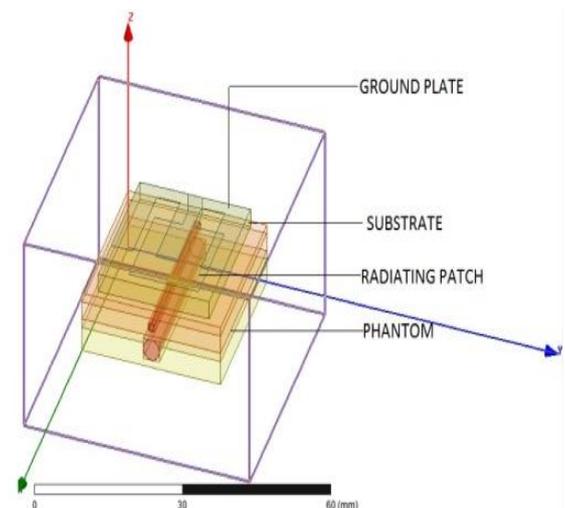


Fig. 5: Wearable Micro Strip Patch Antenna on Normal Vein.

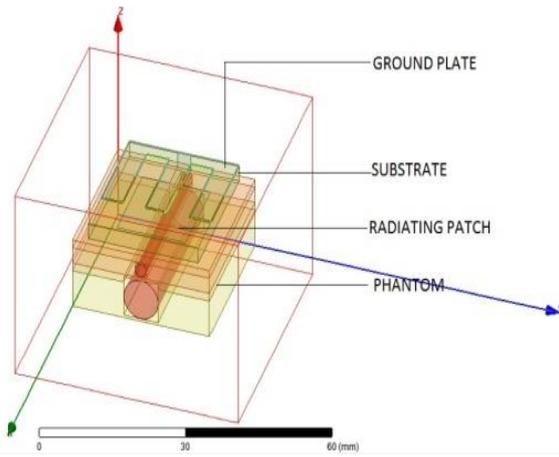


Fig. 6: Wearable Micro Strip Patch Antenna on Varicose Vein.

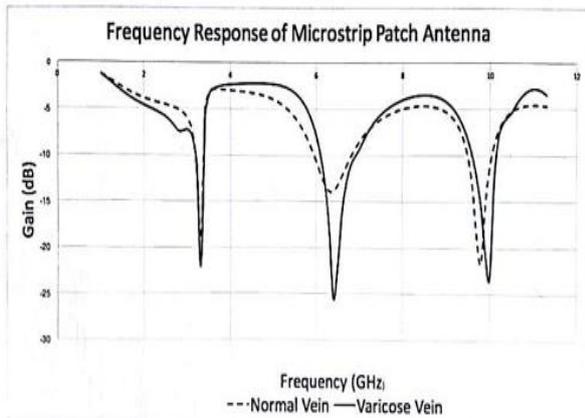


Fig. 7: Frequency Response of the Wearable Micro Strip Patch Antenna.

3.1. Specific absorption rate

Specific absorption rate (SAR) is a measured as the rate of energy that is a absorbed by the human body when exposed to a radio frequency (RF) electromagnetic radiation.SAR is usually averaged either over the whole body or over a small sample of tissue (typically 1g or 10g of tissue). Its unit is W/kg. The formula for SAR is given below,

Equation 6 Specific Absorption Rate

$$SAR = \frac{1}{V} \int_{\text{sample}} \frac{\sigma(\mathbf{r})|\mathbf{E}(\mathbf{r})|^2}{\rho(\mathbf{r})} d\mathbf{r}$$

3.2. Temperature

It is the amount of heat absorbed by the tissue for a particular time period. Its unit is °C. The amount of heat required to penetrate electromagnetic waves in the tissue is 45°C. The temperature for a short period of time (fig.8) and a long period of time (fig.9) are given in formula below,

Equation 7 Temperature

$$\Delta T = SAR \cdot \frac{\Delta t}{c}$$

$$T_{max} = \frac{q}{\lambda'} [1 - (\sqrt{\lambda'} A + 1)e^{-\sqrt{\lambda'} A}]$$

where,

$$q = \frac{\rho S}{K}, \lambda' = \frac{w c_b}{K}; A = \frac{\lambda}{4}$$

3.3. Time period

The duration for which the electromagnetic waves have been penetrated to the tissue to acquire a temperature of 45°C. Its unit is seconds (sec).This can be changed by varying the power level for a given tissue.

3.4. Power level

Power is the rate at which electromagnetic energy is generated or consumed in a particular time period. It is measured in Watts (W). The power conversion is given in the formula below, Equation 8 Power Level

$$1 W = 1 \frac{J}{s} = 1 \frac{N \cdot m}{s} = 1 \frac{kg \cdot m^2}{s^3}$$

3.5. Analysis of normal vein

The SAR Distribution is shown in fig.10 and the various SAR distributions for various power levels are tabulated in Table V.

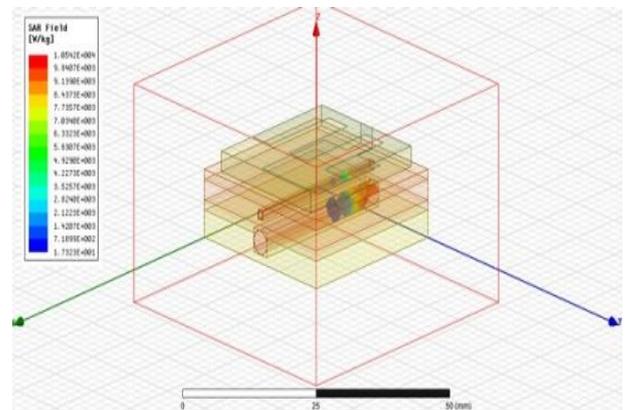


Fig. 8: SAR Distribution Normal Vein.

Table 5: SAR Distribution of Normal Vein

S. No.	SAR (W/Kg)	Temperature (°c)	Power (W)	Time (S)
1.	2108.5	45.311	10	75
2.	4216.9	44.993	20	38
3.	6325.4	45.310	30	25
4.	8433.9	45.311	40	18.75
5.	10542	45.309	50	15

3.6. Analysis of varicose vein

The SAR Distribution is shown in fig.11 and the various SAR distributions for various power levels are tabulated in Table 6.

Table 6: SAR Distribution of Varicose Vein

S. No.	SAR (W/Kg)	Temperature (°c)	Power (W)	Time (S)
1.	2618.7	45.349	10	73
2.	5237.3	45.019	20	30
3.	7856	45.020	30	20
4.	10475	45.028	40	15
5.	13093	45.037	50	12

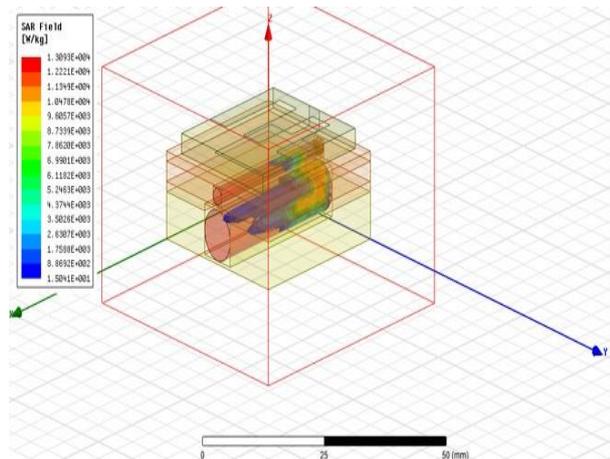


Fig. 9: SAR Distribution Varicose Vein.

4. Discussions

As the SAR increases in the saphenous veins, the temperature also increases. This is because of the fact that the increasing amount of radiation in the tissue causes heating at a faster rate. When the amount of heat in the tissue is higher, the time required to regain

the elasticity of the collagen in the saphenous vein will also increase. The amount of heat transferred into a tissue (per kg) is the SAR (average) of the saphenous vein. As the density of the tissue increases, the power level of tissue will tend to decrease. Table VII shows the observations between normal and varicose veins for the various parameters that have been analysed.

5. Conclusion

In this varicose vein therapy, using finite element analysis, an antenna is sketched out as a wearable micro strip patch antenna. Antenna controls the heat that radiates to the tissue. The tissue is heated then the size of the varicose vein is reduced and the vein is straightened. The results of simulation and analysis by using ANSYS HFSS 17.2 software- the microwave frequency is defined to 9.8 GHz with SAR distribution is 13093 W/kg to obtain a temperature of 45.037°C and the time taken for the antenna to achieve this temperature is 12 seconds. Varicose vein therapy by using microwave ablation is a new surrogate manoeuvre for the patient and hopefully may reduce the use of medicines and help in varicose vein treatment in the future.

Table 7: SAR Distribution, Temperature and Time for Normal and Varicose Veins for Various Power Levels

Power Level (W)	Sar Normal Vein (W/Kg)	Sar Varicose Vein (W/Kg)	Temp Normal Vein(°C)	Temp Varicose Vein(°C)	Time Normal Vein (S)	Time Varicose Vein(S)
10	2108.5	2618.7	45.311	45.349	75	73
20	4216.9	5237.3	44.993	45.019	38	30
30	6325.4	7856	45.310	45.020	25	20
40	8433.9	10475	45.311	45.028	18.75	15
50	10542	13093	45.309	45.037	15	12

References

- [1] S. Prasantamrongsiri, P. Phasukkit, C. Pintavirooj, S. Tungjitkusolmun, A.Sanpanich, "3D Finite Element Analysis for Varicose Vein Therapy by Using Microwave Ablation", The 2012 Biomedical Engineering International Conference (BMEiCON-2012). <https://doi.org/10.1109/BMEiCon.2012.6465480>.
- [2] Tamar Nijsten, Renate R. van den Bos, Mitchel P. Goldman, Michael A. Kockaert, Thomas M. Proebstle Eberhard Rabe, Neil S. Sadick, Robert A. Weiss, Martino H.A. Neumann, "Minimally invasive techniques in the treatment of saphenous varicose veins", JAAD. 2009; 60:110-9. <https://doi.org/10.1016/j.jaad.2008.07.046>.
- [3] S SUBRAMONIA, TA LEES, "The treatment of varicose veins", Ann R Coll Surg Engl 2007.s
- [4] Stephen J Goodyear, Isaac K Nyamekye, "Radiofrequency ablation of varicose veins: Best practice techniques and evidence", 2015, Vol. 30(2S) 9-17 Phlebology.
- [5] M A Anwar, T R A Lane, A H Davies, I J Franklin, "Complications of radiofrequency ablation of varicose veins", 2012; 27 Suppl 1:34-39 Phlebology.
- [6] Chaitali Ingale, Trupti Ingale, Anand Trikolikar, "Study of Different Types of Microwave Antenna and Its Applications", Special Issue, March-April 2013, Volume-3.
- [7] Eng Gee Lim, Zhoa Wang, Jing Chen Wang, Mark Leach, Rong Zhou, Chi-un Lei, Ka Lok Man, Wearable Textile Substrate Patch antennas, IEEE
- [8] Liton Chandra Paul, Nahid Sultan, Design Simulation Performance Analysis of a Line Feed rectangular Microstrip Patch Antenna, International Journal of Engineering Sciences & Emerging Technologies
- [9] <https://www.everythingrf.com/rf-calculators>
- [10] <https://www.pasternack.com/t-rf-microwave-calculators-and-conversions.aspx>
- [11] Varshini Karthik, T.Rama Rao, Investigations on SAR and Thermal Effects of a Body Wearable Microstrip Antenna, Springer 2017.
- [12] T. Padmapriya and V.Saminadan, "Improving Performance of Downlink LTE-Advanced Networks Using Advanced Networks Using Advanced feedback Mechanisms and SINR Model", International Conference on Emerging Technology (ICET), vol.7, no.1, pp: 93, March 2014.
- [13] S.V.Manikanthan and T.Padmapiya "Recent Trends In M2m Communications in 4g Networks and Evolution towards 5g", International Journal of Pure and Applied Mathematics, ISSN NO: 1314-3395, Vol-115, Issue -8, Sep 2017.
- [14] N Bala Dastagiri, K Hari Kishore "Novel Design of Low Power Latch Comparator in 45nm for Cardiac Signal Monitoring", International Journal of Control Theory and Applications, ISSN No: 0974-5572, Vol No.9, Issue No.49, page: 117-123, May 2016.