

Automated target controlled anaesthesia injector

Sri Vidhya Lakshmi.S^{1*}, Andrews Luxcy. E¹, Vishnupriya. U¹, Bhargavi Haripriya. A²

¹Final year, Biomedical Engineering Department

²B.E, M.S Assistant Professor, Biomedical Engineering Department SRM Institute of Science and Technology

*Corresponding author E-mail: vidhyaswaminathan.1996@gmail.com

Abstract

Anaesthesia plays a vital role in major operations which lasts for longer duration of time. The anaesthetic condition of a patient is determined by an anaesthetist based on the body conditions and feed the amount of anaesthesia to be delivered into a modern anaesthesia machine, which delivers the drug as instructed. If a patient experience a sudden change in the body condition where the instructed anaesthesia level cannot help, the anaesthetist and doctors will face severe problems during the operation which leads to patient awakening or may even cause death. So, the patient's body condition has to be continuously monitored and the anaesthesia dosage has to be delivered based on the changes in the body condition. This requires an automated operation of anaesthesia injector which works based on the changes in the patient's body condition by monitoring the vital parameters by itself. This can avoid over dosage and its side effects, eventually reduces the death rate caused by the improper administration of Anaesthesia. Initially, certain amount of dosage is delivered by the anaesthetist based on the patient's condition and earlier reports. Then, during the surgery the anaesthesia is administered if required by this 'Automated Target Controlled Anaesthesia Injector'. Our idea is to monitor the necessary body parameters like temperature, blood pressure, and heart rate by the sensors interfacing it to the microcontroller-PIC16f877a and programmed to deliver the dosage level using stepper motor based on the changes in the parameters. Though, there are so many ideas on automated operation of anaesthesia injector using different micro-controllers and microprocessor, the revolution made in this idea is to use PIC Microcontroller which has an advantage of in-built amplifier, analog to digital convertor & EEPROM coupling with the vital parameters determining the dosage to be administered and assistive mobile-app which helps to reduce the work of anaesthetist by monitoring even from distant places.

Keywords: Use about five key words or phrases in alphabetical order, Separated by Semicolon.

1. Introduction

Every year, 954 surgeries per day take place in India [12]. General Anaesthesia produces unconsciousness and affects your whole body. Regional anaesthesia affects a portion of your body. Local anaesthesia medications are used in many dental procedures, diagnostic tests and some surgeries. They do not cause unconsciousness and are less risky than general anaesthesia. Conscious sedation medications may be given in addition to local anaesthesia to relax you during a procedure and block memory. Local numbing agents allow you to remain awake and alert while deadening feeling in a small area of your body. Some of the more common side effects that could indicate an anaesthesia overdose are Nausea or vomiting, Respiratory distress, Hypothermia, Hallucinations, Seizures, Mental or physical impairment, Dementia, Prolonged unconsciousness, Brain injuries and even Death.

During the surgery, anaesthetic condition of a patient is highly essential. An anaesthetist plays a key role in observing the earlier reports and body conditions of the patient for assisting the anaesthesia dose. Anaesthesia cannot be given completely to a patient in a single stroke, which may cause severe side effects and even leads to death. There are also high chances of patient awakening in-between the surgery, if the dosage delivered is low.

Hence, the dosage of anaesthesia should be administered to a patient based on observing earlier reports by the anaesthetist before undergoing the surgery and also deliver whenever there are changes found in the body parameters during the surgery which will be a difficult task for an anaesthetist.

To overcome the difficulties faced by the Anaesthetist, An automated operation of anaesthesia injector is highly encouraged by anaesthetists.

The anaesthesia dose to be delivered during the surgery is based on the changes in body conditions of the patient which can be observed by monitoring the vital parameters. The important parameters by which the dosage can be determined are Body temperature, Heart-Rate and Blood pressure. So, The Anaesthesia Injector has to work based on the changes in the vital parameters of the patient to deliver accurate amount of dosage. This can absolutely avoid death rate caused by over dosage of anaesthesia and also its side effects.

This project is into automated operation of Anaesthesia Injector by monitoring the vital parameters of the patient which requires a Heart-beat sensor, Temperature sensor, Blood pressure sensor and an interface PIC microcontroller to couple the sensors and the injector operation. This idea is also into developing an assistive Mobile-app which provides user friendly interface to the anaesthetist. Suppose if an anaesthetist is an emergency to assist two or more surgery at the same time, he can monitor all the three surgery at his mobile and attend the one he is require to.

The revolution made in this idea is to use PIC Microcontroller which has an advantage of in-built amplifier, analogue to digital convertor & EEPROM coupling with the vital parameters determining the dosage to be administered and assistive mobile-app. This paper further explains the Working of the system with Block diagram description, Measurement of biomedical parameters, PIC as an interface, System architecture which includes hardware implementation and component selection.

2. Objectives

Objectives of this prototype include:

- A working model of automated anaesthesia injector used for a patient during the surgery.
- To deliver accurate amount of dosage to the patient automatically by monitoring the vital parameters which will avoid over dosage and its side effects.
- To gain wide knowledge in embedded systems, which makes it to work very compactly.
- To develop an assisting mobile app which provides user friendly interface to the anaesthetist.

3. Working of the system

3.1. Block diagram description

The below mentioned block diagram represents the working of the automated target controlled anaesthesia injector. By using the default value provided along with the Microcontroller, the anaesthetist can set the level of anaesthesia to be administered to the patient in terms of milli-litres per hour. It analyses various vital parameters from the various sensors. Then it determines the direction of rotation of DC motor. The rotation of DC motor causes the movement of infusion pump either in forward or backward direction and the anaesthesia provided in the syringe is injected into the patient body. Micro controller is programmed with the certain ranges based on patient body condition through which the motor plays the role. If suppose the patient conditions goes above those certain ranges then the motor will run and inject the Propofol which is the general anaesthesia commonly used for all the patients. If the values of vital parameters goes below the given range then motor stops running and gives an alarm so as to indicate the anaesthetist, in case of emergency. Micro controller is programmed using two software namely, MPLAB IDE v8.92 and Proteus 8 Professional. Biomedical parameter ranges can be programmed using MPLAB and those programs can be executed using Proteus software. The hardware circuit can also be interfaced with the PC using the TTL cable.

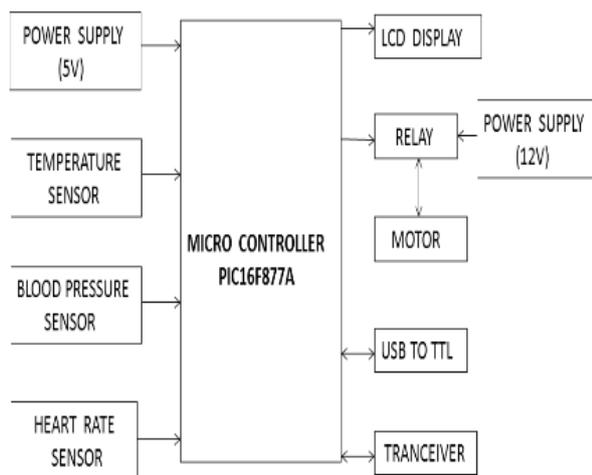


Fig. 1: Block Diagram Representation of the Automated Anaesthesia Injector.

3.2. Measurement of biomedical parameters

In the proposed design, biomedical parameters such as blood pressure, heart rate and temperature are taken into consideration, they depict the patient's overall condition. These are the three vital parameters that are monitored while administering anaesthesia. Biomedical sensors are used in order to measure them, based on the output from these sensors the amount of anaesthesia to be

injected is determined. The whole system functions depend on these parameters, especially the motor. Mostly biomedical sensors are transducers and thermistors which are fabricated in specific forms suitable to use. The sensors used for measuring the vital parameters are, Blood pressure - The normal blood pressure range is 120/80 mmHg, after the injection of anaesthesia the individuals blood pressure may increase or decrease but once the patient becomes unconscious, the blood pressure comes down from the normal range and this condition is termed as hypotension Heart beat - The heartbeat of an unconscious patient is also below the normal rate of 60 to 100 bpm. Photoplethysmography is a technique where the light absorption of the blood vessels in finger tip is taken in consideration to reveal the heartbeat rate, as there will be fluctuation in the reflected light due to the pulsatile flow caused by the heartbeat.

Temperature sensor- The temperature of a patient after anaesthesia administration enters mild hypothermia state but this is very slightly below the normal state of 36 degrees, if the body temperature decreases less than 35 degrees then the anaesthetist is alarmed.

3.3. PIC as an interface

The revolution made in this idea is to use PIC Microcontroller as an interface which has an advantage of in-built amplifier, analog to digital convertor & EEPROM coupling with the vital parameters which helps to determine the dosage to be administered. The blood pressure sensor, temperature sensor, and the heart rate sensor act as inputs to the microcontroller. Basically analogue signals are too weak and of low frequency which is difficult for further processes, so an in-built amplifier is used for amplification. The amplified analogue signal is converted into digital signal by in-built analogue to digital convertor of PIC. Normal range of values for each vital parameter is programmed in the microcontroller and also programmed in such way to run the motor in order to administer the drug when the parameter goes out of the normal range. This PIC microcontroller is chosen as interface as it has got multi-purpose to do with as an in-built amplifier, analogue to digital convertor & EEPROM.

3.4. System architecture

In our proposed system microcontroller plays a key role in executing the output. The sensors which are connected with the microcontroller senses the value of biomedical parameters and read the inputs from the keypad provided with the microcontroller into the software, MPLAB. Proteus software executes the output based on the program which we implemented in MPLAB. The outputs of the circuits is amplified by means of an amplifier and fed into an analog to digital converter. The microcontroller displays the parameters in digital value in the display device. The software is mainly used to burn the programs in MPLAB and will operate in the Proteus. The parameters are checked with their values for every specified interval. These software calculate the stepper motor movement with the parameters provided by the sensors.

3.5. Software implementation

The block diagram is produced in the software by connecting the circuit using the selected components which are available readily in the Proteus 8 Pro. The normal ranges of all the body parameters are fed in the microcontroller along with the conditions to make the motor run when the sensor output goes out of the normal range with the help of algorithm made in the MP Lab software.

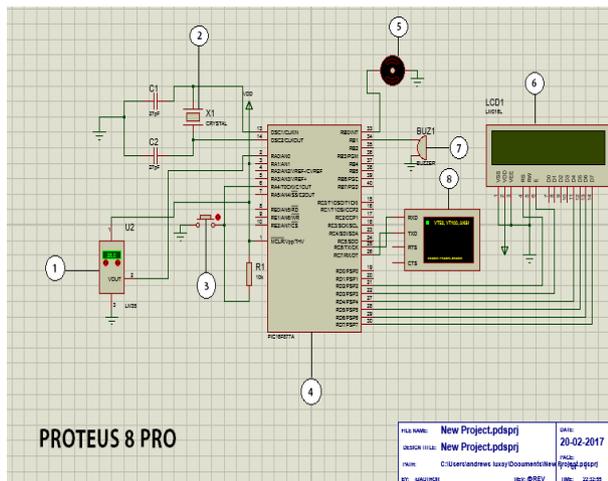


Fig. 2: System Schematic in Proteus 8 PRO.

In FIGURE.2 the labelled parts are,

- 1) Temperature sensor
- 2) Crystal oscillator
- 3) Heart rate sensor
- 4) PIC16F877A
- 5) DC Motor
- 6) LCD Display
- 7) Buzzer
- 8) Blood pressure sensor

The working of the setup is explained in experimental methodology.

Algorithm designed for the functioning of PIC Microcontroller with the help of MPLab:

Step 1: Connect the sensors to the patient

Step 2: Start the automated anaesthesia injector

Step 3: If 'TEMP' is >36 [high]

Output value = 1

(Motor will start rotate to inject the gas)

Step 4: Else if 'TEMP' = < 35 [low]

Output = 0

(Motor off & buzzer on)

Step 5: If 'BP' = >120/80 mm hg [high]

Output = 1.

(Motor will start rotating)

Step 6: Else if 'BP' = <120/80 mm hg [low]

Output=0

(Motor off & buzzer on)

Step 7: If 'HR' = >100 beats/min [high]

Output = 1.

(Motor will start rotating)

Step 8: Else if 'HR' = <60 beats/min [low]

Output = 0.

(Motor off & buzzer on)

3.6. Hardware implementation

The system architecture designed in the software is generated as such in hardware with the same specifications as produced in software. The hardware components are chosen in such a way to be compatible with the PIC microcontroller. The components selection and specifications of the system architecture are listed below.

Components used in automated target controlled Anaesthesia Injector are,

- Regulated power supply (5V and 12V)
- Microcontroller (PIC16F877A)
- Blood pressure sensor
- Heart rate sensor (TCRT1000)
- Temperature sensor (LM35)
- 10rpm 12V DC motor
- LCD display

- USB & TTL.

Regulated power supply

Power supply is the primary component, it consists of a transformer, bridge rectifier and a filter. Voltage regulator IC's such as LM7805 and LM7812 are used in combination with capacitors. The bridge rectifier converts the AC voltage to DC voltage. The main AC voltage of 230V is given to the two step-down transformers, one step-downs 230V to 5V which is used for the PIC microcontroller and the other for converting 230V to 12V for the DC motor, a relay circuit is used in this case to control the power supply. The regulated power supply 5v & 12v circuit board was manufactured in India and supplied by Surya electricals.[13]

Microcontroller (PIC16F877A)

The main component of this idea is PIC-16F877A

It's a 40-pin 8-bit CMOS FLASH microcontroller.

It has two types of internal memories: program memory and data memory. Program memory is provided by 8K words of flash memory. Data memory has two sources: One type of data memory is 368byte RAM, and other is 256byte

This microcontroller acts as an interface between biomedical parameter sensors and the output to be delivered. Pic microcontroller 16f877a used is supplied by India mart which is manufactured in India.[14]

Blood pressure sensor

The normal blood pressure range is 120/80 mmHg, after the injection of anaesthesia the individuals blood pressure may increase or decrease but once the patient becomes unconscious, the blood pressure comes down from the normal range and this condition is termed as hypotension. The transducer used for measuring blood pressure is the common ones that are found in the multiparameter monitors which contains the standard cuff and pump, this setup is connected to a pressure sensor that measures the patient's blood pressure and sends it to the pic microcontroller. When there is any change or increase in the patient's blood pressure then the system is designed to alert the anaesthetist and the motor runs to administer anaesthesia in case of high blood pressure which indicates the patient is regaining his/her consciousness.

Heart beat sensor

The heart beat sensor used here is TCRT1000, it is a reflective optical sensor which works on the principle of photoplethysmography. The heartbeat of an unconscious patient is also below the normal rate of 60 to 100 bpm. The motor runs when the heart beat is above normal range as it indicates the patient is awake. Photo plethysmography is a technique where the light absorption of the blood vessels in finger tip is taken in consideration to reveal the heartbeat rate, as there will be fluctuation in the reflected light due to the pulsatile flow caused by the heartbeat. In TCRT1000 there are two optical components an IR or LED emitter and detector, both are placed on the same side of the finger as it follows reflective technology, the whole system is packed in a light blocking package to avoid wrong output. Heart rate sensor TCRT1000 was made in India supplied by SRI electronics, embedded solutions. [15].

Temperature sensor

The temperature of a patient after anaesthesia administration enters mild hypothermia state but this is very slightly below the normal state of 36 degrees, if the body temperature decreases less than 35 degrees then the anaesthetist is alarmed. The temperature sensor used is LM35 is a linear integrated circuit which gives its output directly in Celsius scale which reduces further calculations as if it is Kelvin then subtraction of large numbers are involved. Temperature sensor LM35 was made in India supplied by amazon with the model robokart. [16]

DC motor-10RPM 12V with Gearbox

The features of this DC motor are 3000RPM base motor, 6mm shaft diameter with internal hole, 125gm weight, Same size motor available in various rpm, 12kgcm torque, No-load current = 60 mA(Max), Load current = 300mA(Max). The motor runs, instructed by the PIC microcontroller when it finds changes in the normal range of parameter values. DC motor was manufactured in

- [7] Microcontroller and their applications- Kenneth J.Ayalaa – Pen ram International.
- [8] David A Bell “Electronic Devices & Circuits”
- [9] Temperature sensor, <http://www.electronicshobby.com/2014/11/temperature-monitor-using-pic16f877a.html> accessed on 11th January, 2018
- [10] LCD Display, <https://electrosome.com/lcd-pic-mplab-xc8/> accessed on 11th January, 2018
- [11] Complications of anaesthesia, <https://www.bakerandgilchrist.com/medical-malpractice-lawyer/complications-of-general-anesthesia/> accessed on 11th January, 2018
- [12] Surgeries in India, <https://data.worldbank.org/indicator/SH.SGR.PROC.P5?end=2012&locations=IN&start=2012&view=chart&year=2015> accessed on 11th January, 2018
- [13] Regulated power supply, <https://www.flipkart.com/surya-el-5v-12v-regulated-power-supply-board/p/itmepmwgbz6ex3zn> accessed on 11th January, 2018.
- [14] PIC Microcontroller, <https://dir.indiamart.com/search.mp?ss=pic+microcontroller+board+16f877a&src=as-context%3Akwd%3Dpic+microcontroller> accessed on 11th January, 2018
- [15] Heart beat sensor, <https://dir.indiamart.com/impcat/heart-beat-sensors.html> accessed on 11th January, 2018
- [16] Temperature sensor, <https://www.amazon.in/LM-35-Temperature-Sensor-Robokart/dp/B00ZNCBQ9O?tag=googinhydr18418-21&tag=googinkenshoo-21&ascsubtag=d3fb631b-b2d1-412d-b343-730e4074b6bc> accessed on 11th January, 2018
- [17] Motor, <https://www.amazon.in/10-RPM-Geared-Motor-Robokart/dp/B010V2JX68> accessed on 11th January, 2018
- [18] USB to TTL cable, https://www.ebay.in/itm/6Pin-FTDI-FT232RL-USB-To-Serial-Adapter-Module-USB-TO-TTL-RS232-Arduino-Cable-/222771214743?_trksid=p2059707.m48543.l9013, accessed on 11th January, 2018.